

UltraSafe

# UltraSafe® Passive Delivery System vs. BD Preventis™



Order  
here

# UltraSafe® Passive™ Delivery System vs. BD Preventis

## Objectives




- Compare two 510K cleared products - the UltraSafe Passive Delivery System and the BD Preventis
- Determine usability, acceptability and preference

## Study Design

- Face-to-face interviews; 35 nurses in three US metropolitan areas
- Rotating devices, after demonstration opinions and preference data
- Secondary study - 10 nurses - Unaided research - no demonstration gathering opinions and preferences

## Key Results

- UltraSafe Passive scored higher on ALL subjective criteria queried
- 94.3% of nurses preferred UltraSafe Passive over BD Preventis In “Unaided” portion
- All nurses preferred UltraSafe Passive and ALL nurses able to activate appropriately with no training
  - NONE of the nurses activated BD Preventis without training

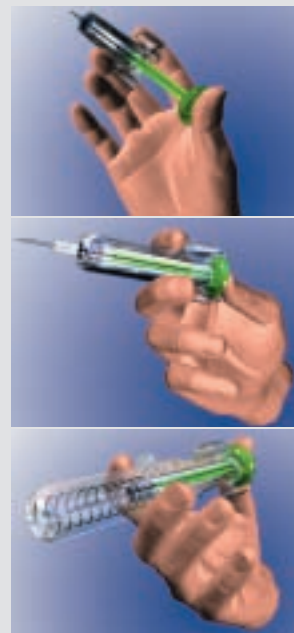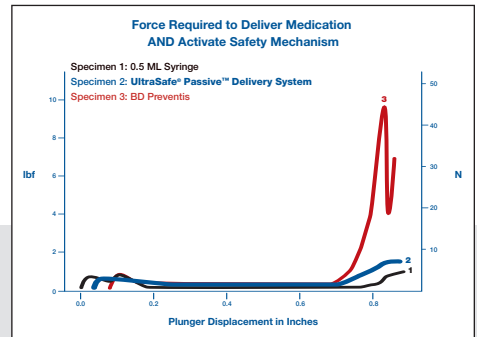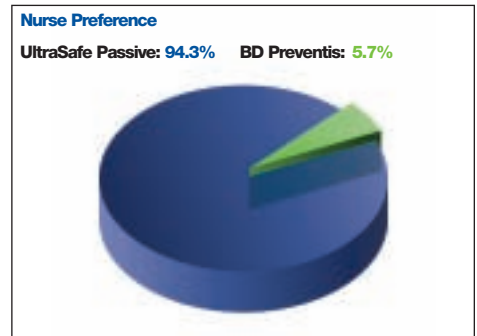

The Tamper Evident UltraSafe® Passive™ Delivery System – One-handed, Patented, Passive activation with an integral tamper evident feature

Go see the action!  
[www.safetysyringes.com](http://www.safetysyringes.com)

**UltraSafe®**  
Delivering Safety Solutions®

**Safety Syringes, Inc.**  
Corporate Headquarters  
Carlsbad, CA  
760.918.9908  
Fax 760.918.0565  
[www.safetysyringes.com](http://www.safetysyringes.com)

UltraSafe®, UltraSafe Passive™ and Delivering Safety Solutions® are trademarks of Safety Syringes, Inc. Carlsbad, CA USA. Products covered by one or more US Patents 6030366, 6159184, 6171283, 6344032, 6416323, 6613022, 6623459 and RE 37439; other patents pending. 0000255 Rev. A